

Produkte
Products

Prüfbericht - Nr.: <i>Test Report No.:</i>		CN25IYGM 001		Seite 1 von 15 <i>Page 1 of 15</i>	
Auftraggeber: <i>Client:</i>		Mettler-Toledo (Changzhou) Precision Instruments Ltd. 22 Zhengqiang Road, Xinbei District, Changzhou, 213022 Jiangsu, P.R. China			
Gegenstand der Prüfung: <i>Test item:</i>		Weighing Terminal			
Bezeichnung: <i>Identification:</i>		IND360 Version: Panel / IND360 Version: Harsh		Serien-Nr.: <i>Serial No.:</i> Engineering samples	
Wareneingangs-Nr.: <i>Receipt No.:</i>		180349991		Eingangsdatum: <i>Date of receipt:</i> 2025-10-22	
Zustand des Prüfgegenstandes bei Anlieferung: Condition of test item at delivery:				Good for testing and checking	
Prüfort: <i>Testing location:</i>		TÜV Rheinland / CCIC (Ningbo) Co., Ltd. 3F Building C13, R&D Park, No. 32, Lane 299 Guanghua Road, National Hi-Tech Zone, Ningbo, 315048, P.R.China			
Prüfgrundlage: <i>Test specification:</i>		NEMA 250-2020			
Prüfergebnis: <i>Test Result:</i>		Der Prüfgegenstand entspricht oben genannter Prüfgrundlage(n). <i>The test item passed the test specification(s).</i>			
Prüflaboratorium: <i>Testing Laboratory:</i>		TÜV Rheinland / CCIC (Ningbo) Co., Ltd. 3F Building C13, R&D Park, No. 32, Lane 299 Guanghua Road, National Hi-Tech Zone, Ningbo, 315048, P.R.China			
Geprüft/ Tested by:			Kontrolliert/ Reviewed by:		
 2025-12-19 Ethan Chen / Shuofeng He			 2025-12-22 Zeke Jia		
Datum <i>Date</i>	Name <i>Name</i>	Unterschrift <i>Signature</i>	Datum <i>Date</i>	Name <i>Name</i>	Unterschrift <i>Signature</i>
Sonstiges/ Other Aspects:					
1. This report issued for NEMA 250-2020 – Type 4 & Type 12 test specification. 2. The test result of this report is only related to specimens received.					
Abkürzungen: P(ass) = entspricht Prüfgrundlage F(ail) = entspricht nicht Prüfgrundlage N/A = nicht anwendbar N/T = nicht getestet			Abbreviations: P(ass) = passed F(ail) = failed N/A = not applicable N/T = not tested		
Dieser Prüfbericht bezieht sich nur auf das o.g. Prüfmuster und darf ohne Genehmigung der Prüfstelle nicht auszugsweise vervielfältigt werden. Dieser Bericht berechtigt nicht zur Verwendung eines Prüfzeichens. <i>This test report relates to the a. m. test sample. Without permission of the test center this test report is not permitted to be duplicated in extracts. This test report does not entitle to carry any safety mark on this or similar products.</i>					

Report Reference No.: CN25IYGM 001

TEST REPORT NEMA 250-2020 Enclosures for Electrical Equipment (1000 Volts Maximum)	
Report Reference No	See cover page
Tested by (printed name and signature)	See cover page
Approved by (printed name and signature)	See cover page
Date of issue	See cover page
Testing Laboratory Name	See cover page
Address	See cover page
Testing location	See cover page
Address	See cover page
Applicant's Name	See cover page
Address	See cover page
Test specification	
Standard	See cover page
Test procedure	N/A
Non-standard test method	N/A
Test Report Form No.	N/A
TRF originator	TUV Rheinland (Shenzhen) Co., Ltd.
Master TRF	Dated May 2024
Test item description	Weighing Terminal
Trademark	METTLER TOLEDO METTLER TOLEDO
Manufacturer	Mettler Toledo (Changzhou) Measurement Technology Co., Ltd. No. 111, West Taihu Road, Xinbei District, Changzhou, Jiangsu Province 213125 China
Factory	Mettler Toledo (Changzhou) Measurement Technology Co., Ltd. No. 111, West Taihu Road, Xinbei District, Changzhou, Jiangsu Province 213125 China

Report Reference No.: CN25IYGM 001

General remarks

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.
 "(see Enclosure #)" refers to additional information appended to the report.
 "(see appended table)" refers to a table appended to the report.
 Throughout this report a point is used as the decimal separator.

Summary of testing:

According to NEMA 250-2020 and product construction, for enclosure Type 4 & Type 12 made of stainless steel, only below test conducted.:

Clause	Test requirement
5.5.2.1	Indoor circulating dust test
5.6	External icing test
5.7	Test for protection against ingress of water (hosedown)
5.8	Indoor corrosion protection
5.9	Outdoor corrosion protection
5.14	Gasket material tests

Particulars: test item vs. test requirements

Equipment mobility: Fixed
 Operating condition.....: Continuous
 Mass of equipment (kg): N/A

Test case verdicts

Test case does not apply to the test object : N/A
 Test items meet the requirement: P(ass)
 Test items do not meet the requirement: F(ail)

Testing

Date of receipt of test item: 2025-10-22
 Date(s) of performance of test: 2025-11-04 ~ 2025-11-20

General product information:

1. These products are weighing terminals, suitable for indoor and outdoor use, the enclosure rating is Type 4 & Type 12.
2. The entire enclosure is constructed of 304 stainless steel, with the top cover secured to the bottom enclosure via threads and sealing gaskets, no conduit opening.
3. During the test, the end of the gland bushing was sealed by 304 stainless steel cover with a short wire.
4. All models in this report have been tested and evaluated based on NEMA 250-2020 standard requirements.
5. Model IND360 Version: Panel was mounted on a steel box used to simulate actual usage scenarios during the test.
6. This report is only issued for tests, the construction safety shall be evaluated additionally by other requirements.

Electrical Rating	
Model Name	Rating
IND360 Version: Panel	24Vdc, 0.8A or 100-240Vac, 50~60Hz, 0.2A
IND360 Version: Harsh	24Vdc, 0.8A or 100-240Vac, 50~60Hz, 0.2A

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7	Construction		P
7.1	Polymeric materials		N/A
7.1.1	Polymeric materials exposed to direct sunlight used for Types 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 6, and 6P enclosures or polymeric materials used for fastenings and/or hinges for these enclosure types shall comply with the Ultraviolet light exposure test (Weatherometer test) specified in Annex B, Ref. No. 1.		N/A
7.1.2	Polymeric materials used for Types 6 and 6P enclosures or polymeric materials used for fastenings and/or hinges for these enclosure types shall comply with the Water exposure and immersion tests specified in Clause 8.16.		N/A
7.1.3	A polymeric observation window necessary to maintain Enclosure Types 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 6, and 6P ratings and secured by an adhesive exposed to direct sunlight shall be conditioned in accordance with the Ultraviolet light exposure test (Weatherometer test) specified in Annex B, Ref. No. 1 prior to investigation of critical property values in accordance with Annex B, Ref. No. 1, or Annex E.		N/A
	Note: This does not apply to adhesives internal to the enclosure where direct sunlight is shielded.		N/A
7.1.4	In Canada, a material used for an observation window shall be mechanically secured or shall be secured using an adhesive complying with Annex E.		N/A
7.2	Corrosion protection		P
7.2.1	General		P
7.2.1.1	Enclosures made of the following materials shall be considered to comply with the indoor and outdoor corrosion requirements:		P
	a) Copper, aluminum, or stainless steel; and	304 Stainless steel	P
	b) Bronze or brass, either of which containing at least 80 percent copper.		N/A
	Note: The materials in (a) and (b) above are not considered to comply with additional corrosion protection of Clause 7.2.4 without being investigated to the requirements of Clause 7.2.4.		P
7.2.1.2	Enclosures shall not be constructed of metals in any combination such as to cause galvanic action that will adversely affect any part of the equipment exposed to moisture.		P
7.2.1.3	Fasteners and hinges used on an enclosure shall be resistant to corrosion and shall comply with the same requirements as the enclosure. Brass inserts containing at least 60 percent copper shall be considered to comply with the indoor and outdoor corrosion requirements.		P
7.2.1.4	Other than as permitted by Clause 7.2.1.5, both the inside and outside surfaces of an enclosure made of ferrous material, along with any external ferrous parts attached to these enclosures, shall be protected against corrosion in accordance with Clause 7.2.2, 7.2.3, or 7.2.4.		N/A
7.2.1.5	The corrosion protection requirement does not apply to:		N/A
	a) Bearings, sliding surfaces of a hinge or shaft, and the like, located on the exterior of these enclosures;		N/A
	b) Sheared or cut edges and punched holes of galvanized sheet steel;		N/A
	c) Parts such as a decorative grill, and the like, that are not required to form part of these enclosures.		N/A
7.2.2	Indoor corrosion		P

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7.2.2.1	Type 1, 2, 5, 12, 12K, and 13 ferrous enclosures and external ferrous parts attached to these enclosures either:	Type 12, entire enclosure is constructed of 304 stainless steel	N/A
	a) Shall be protected against corrosion by enameling, painting, galvanizing, or other equivalent means; or		N/A
	b) Shall be tested in accordance with Clause 8.7.		N/A
7.2.3	Outdoor corrosion protection		P
7.2.3.1	Type 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 6, and 6P ferrous enclosures, and external ferrous parts attached to these enclosures shall be protected against corrosion by one of the coatings in Clause 7.2.3.1 (a) – (d) or shall comply with the test requirements of Clause 8.8:	Type 4, entire enclosure is constructed of 304 stainless steel	N/A
	a) Hot-dipped mill-galvanized sheet steel conforming to the coating Designation G90 in Annex B, Ref. No. 2;		N/A
	b) A zinc coating, other than that provided on hot-dipped mill-galvanized sheet steel, uniformly applied to an average thickness of not less than 0.015 mm (0.00061 inch) on each surface with a minimum thickness of 0.014 mm (0.00054 inch); the thickness of coating shall be established by the metallic-coating-thickness test described in Annex B, Ref. No. 3 or No. 13; an annealed coating shall comply with Clauses 7.2.3.3 and 7.2.3.4;		N/A
	c) A zinc coating conforming to Clause 7.2.3.1(c)(1) or 7.2.3.1(c)(2) and having at least one coat of an organic finish of the epoxy or alkyd-resin type or other outdoor paint applied after forming on each surface.		N/A
	1) Hot-dipped mill-galvanized sheet steel conforming to the coating Designation G60 or A60 in Annex B, Ref. No. 2; or		N/A
	2) A zinc coating, other than that provided on hot-dipped mill-galvanized sheet steel, uniformly applied to an average thickness of not less than 0.010 mm (0.00041 inch) on each surface with a minimum thickness of 0.009 mm (0.00034 inch); the thickness of the coating shall be established by the metallic-coating-thickness test described in Annex B, Ref. No. 3 or No. 13.		N/A
	The acceptability of the paint may be determined by consideration of its composition or by corrosion tests if these are considered necessary; or,		N/A
	d) Paint shall comply with the requirements in Clause 8.8 or Annex B, Ref. No. 7.		N/A
7.2.3.2	Type 3X, 3RX, 3SX, 4X, and 6P ferrous enclosures, and external ferrous parts attached to these enclosures, conforming to 7.2.4.1(a) shall be considered to have met the requirements.		N/A
7.2.3.3	An annealed coating on sheet steel that is bent or similarly formed or extruded or rolled at edges of holes after annealing shall be additionally painted in the affected area if the process damages the zinc coating. See Clause 7.2.3.1(b).		N/A
7.2.3.4	If flaking or cracking of the zinc coating at the outside radius of the bent or formed section is visible at 25 power magnification, the zinc coating is considered to be damaged. Simple sheared or cut edges and punched holes are not required to be additionally protected. See Clauses 7.2.3.1(b) and 7.2.3.8.		N/A

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7.2.3.5	A hot-dipped mill-galvanized G90 coating shall not be damaged during handling or fabrication to the extent that the base metal is exposed, other than as allowed by Clauses 7.2.3.6 and 7.2.3.7. See Clause 7.2.3.1(a).		N/A
7.2.3.6	In accordance with Clause 7.2.3.5, uncoated cross-sectional surfaces at cut edges and drilled openings are acceptable.		N/A
7.2.3.7	In accordance with Clause 7.2.3.5, the base metal may be exposed if:		N/A
	a) The maximum width and length of the exposed metal does not exceed the thickness and length of any cut edge on the sheet; or		N/A
	b) The surface has one coat of an organic finish of the epoxy or alkyd-resin type, or other outdoor paint applied after fabrication.		N/A
7.2.3.8	Sheet steel that employs a hot-dipped mill-galvanized G90 coating that is drawn, formed, extruded, or rolled shall be additionally painted with one coat of an organic finish of the epoxy or alkyd-resin type or other outdoor paint in the areas that are affected by a process that damages the coating as determined by the requirement in Clause 7.2.3.4. See Clause 7.2.3.1(b).		N/A
7.2.3.9	An enclosure of cast iron or malleable iron at least 3.2 mm (1/8 inch) thick shall be protected against corrosion by:		N/A
	a) A 0.0038 mm (0.00015 inch) thick coating of zinc, cadmium, or the equivalent, on the outside surface and a visible coating of such metal on the inside surface; or		N/A
	b) One coat of an organic finish of the epoxy or alkyd-resin type or other outdoor paint on each surface. The acceptability of the paint may be determined by consideration of its composition or, if necessary, by Corrosion tests as specified in Clause 8.8.		N/A
7.2.4	Additional corrosion protection		N/A
7.2.4.1	Type 3X, 3RX, 3SX, 4X, and 6P enclosures, and external parts attached to these enclosures, shall be manufactured of:		N/A
	a) Austenitic stainless steel designated as American Iron and Steel Institute (AISI) Type 302, 303, 304, 305, 309, or 316;		N/A
	b) Polymerics; or		N/A
	c) Other materials that have been determined to comply with Clauses 7.2.3 and 8.9.		N/A
7.3	Openings	For model IND360 Version: Harsh	P
7.3.1	General		P
7.3.1.1	Other than as permitted by Clause 7.3.1.2, openings provided in an enclosure shall comply with the tests in Table 2 or Table 6 with these openings unfilled.		P
7.3.1.2	Openings in accordance with Clause 7.3.2, if provided in the test enclosure, shall be filled as intended to maintain the environmental integrity of the enclosure.		N/A
7.3.1.3	Joints for all devices closing openings into the equipment cavity of a Type 12 or 12K enclosure, as well as any door or cover for a Type 12 or 12K enclosure, shall include a gasket in the full length of the joint. The gasket shall comply with the requirements of Clause 8.13.		P
7.3.2	Equipment openings		N/A

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7.3.2.1	Enclosures may be provided with openings that are intended to be closed by field-installed equipment (such as pushbutton switches, door latches, etc.) if these enclosures are marked in accordance with Clause 9.6.		N/A
7.3.3	Drainage openings		N/A
7.3.3.1	Type 2, 3R, and 3RX enclosures shall have provisions for drainage. Drainage openings shall not be less than 3.2 mm in diameter (1/8 inch in diameter) or more than 6.4 mm in diameter (1/4 inch in diameter), unless baffled or provided with a drainage fitting.		N/A
7.3.3.2	For Type 2, 3R, and 3RX enclosures that also meet the requirements of other enclosure types, the drainage openings shall be closed by a removable plug, and instructions shall be provided in accordance with Clause 9.7.1.		N/A
7.3.3.3	Type 2, 3R, and 3RX enclosures that also meet the requirements of other enclosure types need not have drainage holes if the enclosure is provided with instructions in accordance with Clause 9.7.2.		N/A
7.3.4	Mounting openings	No such parts.	N/A
7.3.4.1	For Type 3, 3X, 3S, 3SX, 4, 4X, 6, 6P, 12, 12K, and 13 enclosures, the mounting means shall be external to the equipment cavity or shall comply with Clause 7.3.4.2. For Type 1, 2, 3R, 3RX, and 5 enclosures, the mounting means shall comply with 6.3.4 of Annex B, Ref. No. 10.		N/A
7.3.4.2	In accordance with Clause 7.3.4.1, the mounting means may pass through the enclosure wall into the equipment cavity if it attaches to an intermediate bracket or foot and is tested in accordance with Clause 8.1. The bracket or foot shall then rely on separate mounting hardware to attach it to the building wall. The mounting means shall not have the same mounting hardware both pass through the equipment cavity and attach directly to the building wall.		N/A
7.3.4.3	The mounting means noted in Clause 7.3.4.1 may be provided as a kit if the kit and the marking or instructions are included with the enclosure referencing this kit. The kit may be supplied separately only if the hardware required to maintain the environmental rating of the enclosure is provided.		N/A
7.3.5	Ventilation		N/A
7.3.5.1	An enclosure may be ventilated if the enclosure is tested in accordance with Clause 8.1 and the applicable design tests for the environmental rating(s) of the enclosure in accordance with Table 6.		N/A
7.4	Conduit connection	For model IND360 Version: Harsh	P
7.4.1	General		P
7.4.1.1	Enclosures shall be designed for use with appropriate conductor entry provisions to maintain the specified environmental capability in accordance with Clause 8.1.1 after proper installation.		P
7.4.2	Hubs and fittings		P
7.4.2.1	An enclosure provided without conduit hubs shall be marked in accordance with Clause 9.6.		P
7.4.2.2	A conduit hub or fitting may be shipped separately if the necessary hardware, gaskets, and instructions are provided with either the enclosure or the fitting.		P

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7.4.2.3	For non-metallic enclosures, other than Type 1, designed for or equipped with detachable threaded conduit hubs that are held in a circular opening, such as a single breakout or knockout, pre-punched openings, or user-punched (as specified in the manufacturer's instructions) openings, by means of a locknut or equivalent, shall withstand a Misalignment test in accordance with the requirements of 8.15 applied to any detachable hub installed in the enclosure.		N/A
7.4.2.4	In Canada, the requirements of Clause 7.4.2.3 shall also apply to metallic enclosures, other than Type 1, with wall thickness less than 1.35 mm (0.05 in).		N/A
7.4.3	Knockouts and breakouts		N/A
7.4.3.1	All enclosure types may have knockouts and breakouts, except Type 12 enclosures.		N/A
7.4.3.2	Knockouts and breakouts shall meet the appropriate design tests in Table 2 or Table 6 for the enclosure type in which they are provided.		N/A
7.5	External operating mechanisms		N/A
7.5.1	External operating mechanisms, when mounted on or through the enclosure, shall comply with the applicable design tests in Table 2 or Table 6 for the enclosure type unless otherwise specified.		N/A
7.5.2	External operating mechanisms on a Type 3S and 3SX enclosure shall support the additional weight of ice and withstand the removal of ice by a hand tool. See Clause 8.5.		N/A
7.6	Access to interior		N/A
7.6.1	Types 3, 3X, 3R, 3RX, 3S, 3SX, 5, 12, and 12K enclosures shall require the use of a tool to gain access to the equipment cavity or shall have provisions for locking. When the provision for locking is provided as an accessory:		N/A
	a) The accessory shall be shipped with the enclosure of which it is intended to be installed; and		N/A
	b) Both the accessory and the enclosure shall comply with Clause 9.		N/A
7.6.2	All closing hardware for Type 5, 12, and 12K enclosures shall be captive.		N/A
7.7	Gaskets		P
7.7.1	A gasket of elastomeric or thermoplastic material or a composition gasket utilizing an elastomeric material that is provided on a Type 2, 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 5, 6, 6P, 12, 12K, or 13 enclosure to meet the environmental construction and performance requirements of this standard shall comply with the Gasket test of Clause 8.13.2 or 8.13.5.	Type 4 & 12	P
7.7.2	A gasket provided on a Type 12, 12K, or 13 enclosure shall be oil resistant and shall additionally comply with the Oil immersion test in Clause 8.13.4.	Type 12	P
7.7.3	A gasket shall be secured with adhesive or by mechanical means. The gasket and its securing means shall not be damaged when the joint is opened.		P

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
7.7.4	A cellular (open cell and closed cell) gasket of elastomeric or thermoplastic material or a composition gasket utilizing an elastomeric material which is under periodic compression and that is provided on a Type 2, 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 5, 6, 6P, 12, 12K, or 13 enclosure to meet the environmental construction and performance requirements of this standard shall comply with the Gasket test of Clause 8.13.3. Gaskets under periodic compression are those which are subject to prolonged periods of compression followed by occasional, short periods of relaxation where the seal provided by the gasket may be broken during the life of the application and, after each such occurrence, the gasket is expected to provide the same seal when recompressed. Gaskets that are between parts of the enclosure not intended to be removed under regular use or maintenance are considered to not be under periodic compression.	Compliance 7.7.5	N/A
	Note: Gaskets under doors or covers intended to be opened or removed in the end use would be considered to be under periodic compression.		N/A
7.7.5	Gaskets under continuous compression are not required to comply with the Gasket tests of Clause 8.13.3.	Gasket is continuous compression at the end of the threads.	P
7.7.6	Gaskets made of solid (non-cellular) elastomeric material are not required to comply with the Gasket tests of Clause 8.13.3.	Gasket use Silicone Rubber	P
7.7.7	Gaskets that have an air space which is compressed to create the environmental seal are not required to comply with the Gasket tests of Clause 8.13.3.		N/A
7.8	Factory-applied sealing compounds	No such parts.	N/A
7.8.1	A sealing compound that is factory-applied on a Type 2, 3, 3X, 3R, 3RX, 3S, 3SX, 4, 4X, 5, 6, 6P, 12, 12K, or 13 enclosure and is relied upon to comply with the design tests of this standard shall be applied to the inside cavity of an enclosure, including at joints or seams.		N/A
	Note 1: This requirement, prior to the sealant compound curing or hardening, does not preclude untrimmed seepage through the joints or seams to the enclosure's exterior during the factory application, nor does this requirement preclude factory-applied sealant by encapsulation from the exterior.		N/A
	Note 2: This requirement does not address field-application of sealant compounds in accordance with manufacturer's installation instructions.		N/A
7.8.2	A sealing compound that is provided on a Type 2, 3, 3R, 3S, 4, 4X, 5, 12, or 12K enclosure and is relied upon to comply with the design tests of this standard shall comply with the Sealing Compounds test of Clause 8.17.		N/A

8	Tests		P
8.1	General		P
8.2	Drip test		N/A
8.2.1	Method A		N/A
8.2.2	Method B		N/A
8.2.3	Evaluation		N/A
8.3	Rain test		N/A
8.4	Dust test		P
8.4.1	Outdoor dust test		N/A

Report Reference No.: CN25IYGM 001

UL 50E & CSA C22.2 NO. 94.2			
Clause	Requirement – Test	Result – Remark	Verdict
8.4.2	Indoor dust test	Corresponding to NEMA 250-2020 5.5.2.1 Indoor circulating dust test. No dust entered.	P
8.5	External icing test	Corresponding to NEMA 250-2020 5.6. Enclosure not broken	P
8.6	Hosedown test	Corresponding to NEMA 250-2020 5.7 Test for protection against ingress of water(hosedown). No water entered	P
8.7	Indoor corrosion protection	Corresponding to NEMA 250-2020 5.8. 304 Stainless steel	N/A
8.8	Outdoor corrosion protection	Corresponding to NEMA 250-2020 5.9. 304 Stainless steel	N/A
8.9	Additional corrosion protection for enclosure type 3X, 3RX, 3SX, 4X and 6P		N/A
8.10	Submersion test		N/A
8.11	Pressure test		N/A
8.12	Oil exclusion test		N/A
8.13	Gasket tests	Corresponding to NEMA 250-2020 5.14 Gasket material tests.	P
8.13.1	General		P
8.13.2	Tensile strength and elongation tests	Alternated by 8.13.5	N/A
8.13.3	Compression test		N/A
8.13.4	Oil immersion test		P
8.13.5	Gasket performance after ageing test		P
8.14	Rod entry test		N/A
8.15	Misalignment test		N/A
8.16	Water exposure and immersion		N/A
8.17	Sealing compounds tests		N/A
8.18	High-pressure power wash test		N/A


Report Reference No.: CN25IYGM 001

Photos

Fig 1.
Test Sample 1
Overall view of model IND360
Version: Harsh



Fig 2.
Bottle view – For model
IND360 Version: Harsh

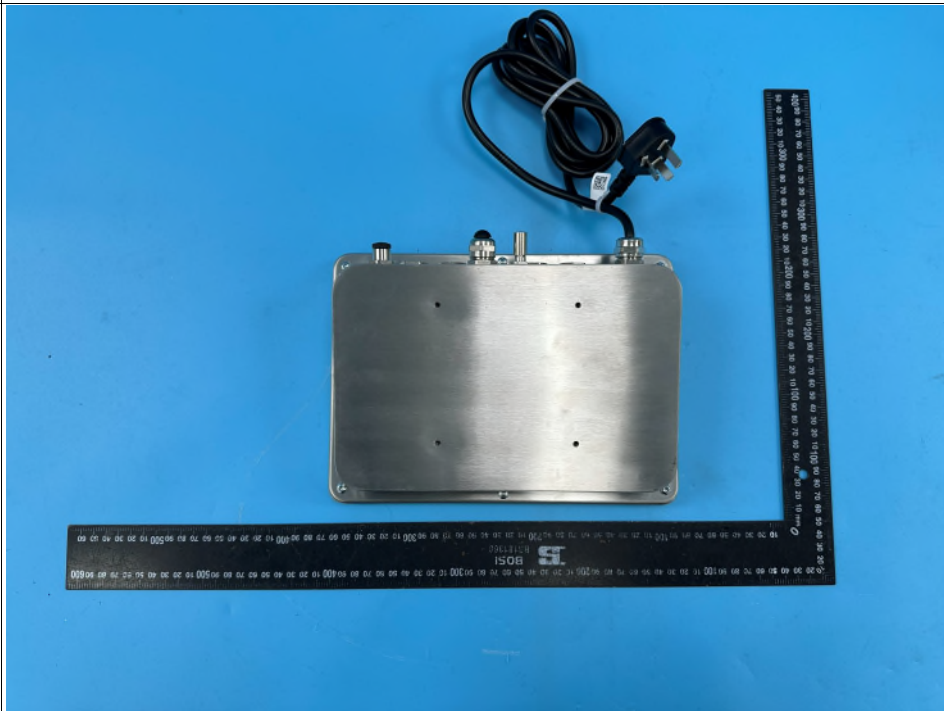

Report Reference No.: CN25IYGM 001

Photos

Fig 3.
Conduit of model IND360
Version: Harsh



Fig 4.
Inside View of model IND360
Version: Harsh



Report Reference No.: CN25IYGM 001

Photos

Fig 5.
Sealing Gasket



Fig 6.
Overall view of model IND360
Version: Panel




Report Reference No.: CN25IYGM 001

Photos

Fig 7.
Sealing Gasket



Fig 8.
Model IND360 Version: Panel
is mounted on the simulation
box

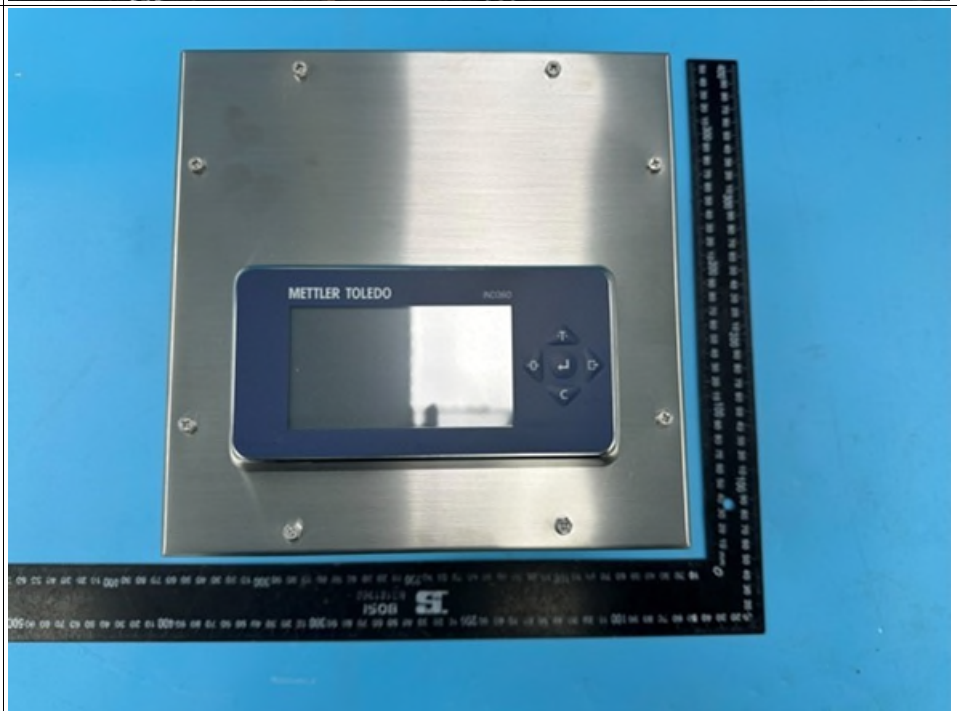

Report Reference No.: CN25IYGM 001

Photos

Fig 9.
Model IND360 Version: Panel
is mounted on the simulation
box



-----End of Report-----